



When crossing profile is critical, the choice is yours

**pRESET** Compatible with 0.021" MC

REF	A: Shaft Diameter [mm]	B: Working Length [mm]	C: Shaft Length [mm]	ID Microcath. [inch]	Min. Vessel Diameter [mm]	Delivery Wire Length [m]
PRE-4-20	4	20	30	0.021	≥ 2	2
PRE-6-30	6	30	48	0.021	≥ 3	2
PRES-5-40	5	40	52	0.021	≥ 2	2
PRES-6-50	6	50	64	0.021	≥ 3	2
PRE-LUX-4-20	4	20	30	0.021	≥ 2	2

FLUOROSAFE MARKER  
2000 mm  
A  
B  
C  
radioopaque  
Fully visible with LUX Technology

**pRESET LITE** Compatible with 0.0165" / 0.017" MC

REF	A: Shaft Diameter [mm]	B: Working Length [mm]	C: Shaft Length [mm]	ID Microcath. [inch]	Min. vessel diameter [mm]	Delivery Wire Length [m]
PRE-LT-3-20	3	20	30	0.0165 / 0.017	≥ 1.5	2
PRE-LT-4-20	4	20	30	0.0165 / 0.017	≥ 1.5	2

FLUOROSAFE MARKER  
2000 mm  
A  
B  
C




See the pRESET in action

Scan the QR-code or visit: <https://goo.gl/bd5hkE>

Continuous commitment to patient care -  
the extended **pRESET** family

A solution for every clot

Backed by clinical evidence

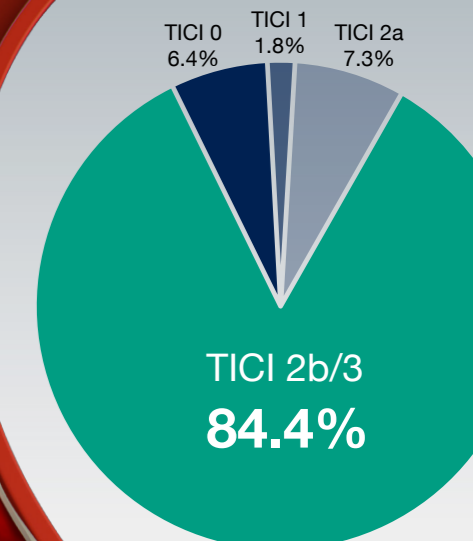

- Unique design elements**
- **Helical slit** maintains cell shape integrity independent of expansion diameter
  - **Closed Ring Design** ensures stable opening and constant wall apposition during retrieval
  - **Dual Type Cell Design** for deep clot integration combined with flexibility in tortuous anatomies


Helical Slit

**pRESET LITE**



- Key features**
- Available as **pRESET LITE** 3-20 and 4-20
  - 0.0165"/0.017" Microcatheter compatible
  - Reach distal clots with **pRESET LITE**

**Best-in-class clot retention and removal of red and white clot**

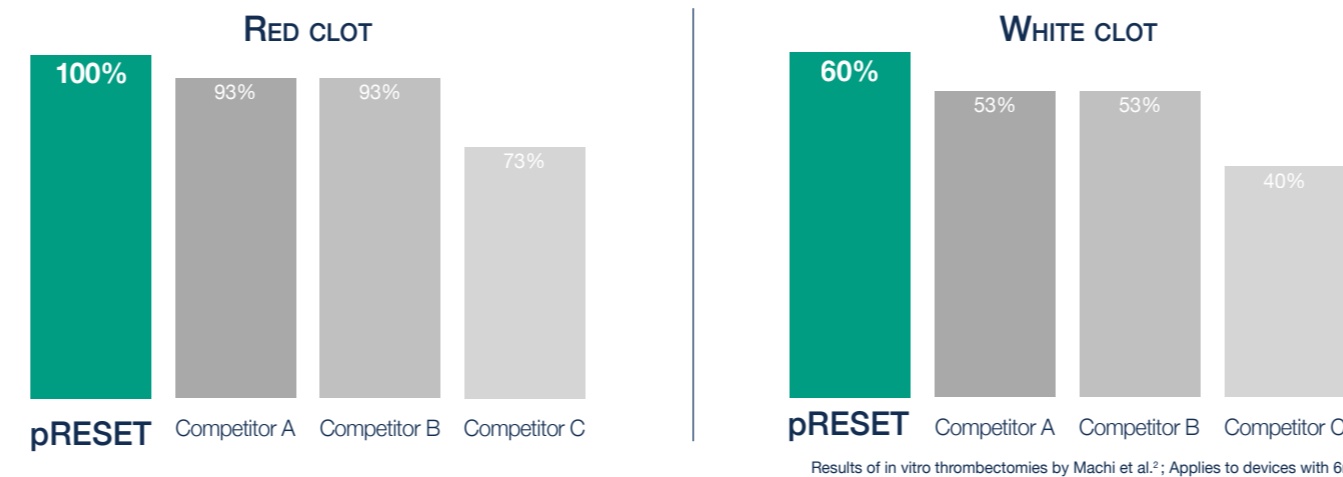

- ARTESp<sup>1</sup> study conclusion**
- Safety and efficacy of mechanical thrombectomy with **pRESET**
  - Excellent recanalization rate
  - Excellent long-term neurological outcome regardless of patient's age

	ARTESp	MR CLEAN	SWIFT-PRIME	EXTEND-IA	ESCAPE
mRS 0-2 90 days	62.5%	32.6%	60%	71%	53%
TICI 2b/3	84.4%	58.7%	88%	86%	73.4%

<sup>1</sup> Prothmann S et al.; Acute Recanalization of Thrombo-Embolic Ischemic Stroke with pRESET (ARTESp): the impact of occlusion time on clinical outcome of directly admitted and transferred patients; J NeuroIntervent Surg 2016; doi:10.1136/neurintsurg-2016-012556.  
<sup>2</sup> Machi P et al.; Experimental Evaluation of Stent Retrievers' Mechanical Properties and Effectiveness; J NeuroIntervent Surg 2016; doi: 10.1136/neurintsurg-2015-012213. Applies for pRESET 6-30.